



# PTCR Technique & Application

## 1. What is a PTCR?

A PTCR is a ceramic device that registers the total amount of heat transferred to it. Because of the advanced technique and materials applied and used for this product, it gives a fair representation of the real heating process taking place in a kiln at the location of the ring. PTCR helps to achieve a reliable, outstanding and regular quality level.

The actual set temperature of a kiln during a firing process, as measured by thermocouples, does not give any guarantee of the repeatability of process conditions which of course will harm the quality of the products. A thermocouple merely gives a specific spot temperature, which is not the same temperature as the one at the position of the product. The ultimate temperature of the product is determined by the total transferred heat. This is not measured by the thermocouple. Besides, the same set temperature in different kilns or kiln layouts does not guarantee the same heat treatment.

The PTCR has been developed to give a better representation of the firing processes to allow a tight control of the real amount of heat transferred, taking into account the above described influences.

The PTCR measures the total heat transferred to the ring, by means of conduction, convection and radiation. It takes into account different firing conditions that may occur in a kiln such as heat sinks, temperature gradients, gasflow, heat transfer coefficient, time, kiln setting, etc. Because of total heat measurement, the repeatability of the process is assured and thus so quality level of the product.



## 2. How does a PTCR work?

The PTCR is a ceramic ring which shrinks if it is exposed to heat. The degree of shrinkage depends on the actual temperature in the kiln, the heat transfer properties of the kiln and the time it is exposed to the heat treatment.

The measured shrinkage is converted by means of a chart into a Ring Temperature (RT) which is an effective temperature that describes the total amount of heat absorbed by the ring and also by the products. The observed Ring Temperature is an effective temperature for the total firing cycle, which has neither direct relation to the absolute temperature in degrees Celsius, Fahrenheit or Kelvin nor any direct relation with the set temperature. The PTCR temperature reading is further influenced by the top temperature hold time (soak time).

At a constant temperature the PTCR will continue to shrink, leading to a higher RT reading. There is a maximum to the hold time, during which the ring will continue to shrink. The maximum hold time, which is typically between 0.5 and 10

hours, depends on the type of ring used and the actual temperature compared to the temperature range of the ring under consideration. Using the PTCR beyond this maximum

hold time may lead to erroneous results because the PTCR ceases to shrink further on a certain moment.



## 3. When to apply PTCR?

Because of its specific properties, PTCR has a wide range of different applications for different purposes. It is a perfect means for the determination and maintenance of the exact heat treatment by the product.

### The main application purposes are

- A) Process control and optimization
- B) Trouble shooting
- C) Yield improvement
- D) Improvement of product quality
- E) Reduction of inspection time and costs
- F) Quality assurance

### A) Process control and optimization

The most frequent use of PTCR is in optimizing and managing the firing processes to arrive at the optimal product quality and to assess the thermal performance and characteristics of a kiln.

The way of working is to make a number of runs with different settings of the parameters temperature and time. These runs are characterised by the RT values as determined from the rings. Product quality analysis determines the optimal run and accompanying RT values. In this way the found Ring Temperature is related to a specific firing process. Once the optimal setting of the process parameters is found, the PTCR is used to control the process and to recognize deviations in time and temperature. In future runs the same RT reading will guarantee the same quality level of the products.

This method is followed whenever a new product or process has to be introduced, to determine differences in the thermal characteristics of new kilns, or after maintenance of kilns.

### B) Trouble shooting

This is one of the traditional applications of PTCR; malfunctioning of (parts of) the equipment. The ring is used to make a mapping of the kiln in RT in order to locate positions with different thermal behaviour.

After root cause analysis proper corrective action can be taken to resolve the problem(s) after the problem is solved. PTCR are used to monitor the thermal performance of the kiln to signal the problem. In the case of monitoring the number of rings of course is smaller than during the analysis phase.

#### C) Yield improvement

Once the mapping of the thermal characteristics is available, one has the possibility to further fine-tune the process settings and optimize the yield. This will also lead to optimization of the energy consumption.

#### D) Improvement of product quality


Because the process is controlled in a much better way, the scatter in the quality of the products is minimised. This means that the quality control of the products can be reduced as a start and may eventually be reduced further to sampling level only or even abandoned completely. Rework (if applicable) will be past tense.

#### E) Reduction of inspection time and costs

The improved processing will allow the reduction of the number of products that have to be inspected and may finally lead to elimination of the product testing completely. The only thing left is the measurement of the rings to monitor the process. Easy measurement can be done by using the PTCR Micrometer which allows only one measurement per ring in order to get a reliable result. In time the sampling rate maybe reduced to a bare minimum, reducing the inspection effort to a minimum, whilst guaranteeing an excellent product quality.

#### F) Quality Assurance

Process control, as formulated in ISO 9001:2000, nowadays can only be achieved by virtue of the availability of an objective means to monitor and control firing processes PTCR provides this objective method.

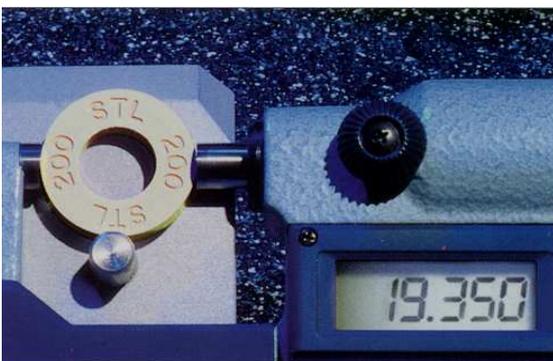

## **4. PTCR Application**

### **4.1. General application advice**

The general procedure during the application is as follows:

#### Step 1) Placement of the rings in the kiln

Select the rings with the right temperature range. The rings have to be placed at any location in the kiln where a determination of the thermal performance is desired. Rings

do not have to be measured before they are put in to place in the kiln because differences are statistically corrected and integrated in the conversion chart.

#### Step 2) Firing process can take place

#### Step 3) Measurement of the rings

After the firing cycle has been terminated, the ring diameters have to be measured. Make sure that the rings are identifiable regarding their position in the kiln for mapping. Every ring only has to be measured once, the special PTCR Micrometer ensures an operator independent, reliable and accurate reading of the ring diameter. In order to assure the reliability the diameters have always to be measured between the two D's.

#### Step 4) Conversion of the diameters into RT

The outer ring diameter can be converted into a Ring Temperature (RT) using the conversion table delivered with every new batch of PTCR. The RT value thus obtained is an accurate representation of the total (cumulative) amount of heat transferred to the products during the temperature cycle.



### **4.2. First time usage**

The first time the PTCR is applied, different (trial) runs with different parameter settings have to be made and the resulting products have to be compared to the quality standard. In this way the optimal process settings and RT values are coupled. In a new run, if the RT values are the same, the firing conditions have been the same and the quality of the product is assured.

It has to be emphasized, that RT values do not necessarily compare to absolute temperatures. Because it measures the heat transferred to the ring, a longer soak time at the same top temperature will cause the ring to shrink further, resulting in a higher RT value. However the PTCR allow you to

accurately determine temperature DIFFERENCE both within and between certain kiln loads and between individual kilns.

The same measured RT values guarantee the same amount of heat transferred. This means that so exactly the same firing conditions have been applied. Relative data in that regard are valid and very useful.

### 4.3. The temperature conversion table

The shrinkage of the diameter of the ring has to be converted in to the Ring Temperature (RT). This table is updated for every batch of rings to be delivered which means that both the product and the conversion table have a unique relation.

By this re-calibration, all possible effects caused by differences in raw material(s) and deviations of green (zero hour) diameter value are compensated for. This ensures the reading of the shrinkage always to result in the same RT value and thus eliminating batch to batch differences for PTCR. This is one of the reasons why the repeatability and reproducibility of the RT readings is very high. It is important to keep in mind that mixing up of tables and PTCR batches leads to false readings of the RT value.

### 4.4. The PTCR Micrometer

The PTCR Micrometer is specially developed for the measurement of the outer diameter of each ring. Because of the unique metal construction on which the Micrometer is attached, each ring has each time exactly the same position. This results in one-time-only measurements while the reliability and accuracy is assured.

Other normal Micrometers can be used for the measurement of the diameter, but this results in less accurate and reliable results. Therefore we strongly advise to invest once in the official PTCR Micrometer.

### 4.5. Interpretation of the Ring Temperature

The main purpose of PTCR is to ensure the repeatability of the firing process and to ensure in this way the constant quality level of the different kiln loads. The Ring Temperature (RT) represents the total amount of heat transferred to the products and thus a constant RT value ensures firing conditions to be identical. The importance of the PTCR is to provide an accurate determination of DIFFERENCES in total heat transferred and to monitor any deviation in the processing conditions. The RT reading has not necessarily a direct relation to the absolute temperature. Under certain conditions RT readings may be related to the absolute temperature scales. The best approximations is obtained by applying a ramp up speed of 120° C/hour and a top temperature hold time (soak time) of 1 hour. The RT reading obtained gives a fair approximation of the absolute temperature with an uncertainty of 10°C.

### 4.6. Different atmospheres

The PTCR originally has been developed for use in heating processes in air. However the ring may be applied under different atmospheric conditions as well provided some rules are taken into account. We advise clients to contact our customer service desk in case of using the rings for firing processes under reductive or vacuum circumstances. In this way the specific advice can be given in order to get optimal results.

As a general rule it can be stated that, under vacuum conditions and reductive atmospheres like N<sub>2</sub>/H<sub>2</sub> mixtures, the ring have to be pre-fired for 2 hours at 600°C to burn out the organic binder system of the ring completely. If this is not done properly, the organic material will not disappear as CO<sub>2</sub>, but will decompose to carbon. This carbon, left behind in the ring, will inhibit the shrinkage of the ring, resulting in a lower RT reading than expected. Under vacuum conditions, the carbon may even precipitate on the kiln wall and contaminate the kiln. Under vacuum too, the RT reading will be lower than expected, because the heat transfer mechanism lacks the contribution of convection.

It is known that PTCR absorb carbon when used in a carbonising atmosphere. The carbon migrates through the ring and will inhibit the shrinkage significantly. It has to be determined by trial and error, to assess whether sufficient shrinkage capability is left to allow an accurate determination of the change in the outer ring diameter.



### 4.7. FAQ

#### 1. What is a PTCR?

PTCR is a ceramic device, which measures the total heat transferred during a firing cycle. It is not a temperature indicator in the same sense as a thermocouple, it is an energy meter. The indicated Ring Temperature is a standard that has to be the same by rehearsed firing processes under the same conditions. In this way the stability of the process and quality of the products is assured.

#### 2. What is the advantage of PTCR over thermocouples?

PTCR measures the thermal conditions at the same place where the product is located, it measures heat instead of a spot temperature. So it measures the true important

parameter for a firing process: the total amount of heat applied to the product.

#### 3. Why is the temperature reading from the PTCR different from the set temperature?

The PTCR measures heat and the reading depends on the set temperature in the kiln and the time the PTCR is exposed to heat.

#### 4. What is the difference between PTCR and its main competitors?

The PTCR allows a numerical determination of the kiln performance and is one of the most reliable products of its kind available on the market. It assures the reproducibility of the heat treatment applied to the product and so it's quality.


Since the ceramic temperature indicator measures heat instead of temperature, the RT reading has no direct relation to the absolute temperature in Celsius or Fahrenheit. Only after taking into account both time and set temperature, a relation between RT value and the Celsius or Fahrenheit scale can be determined.

6. Is there any limitation to the type of kiln, where PTCR can be applied?

No, PTCR can be applied in all kinds of kilns used in the industry.

7. Can PTCR be used in every atmosphere?

In principle yes. However in case of reducing atmospheres or vacuum conditions, the LT and ST versions of PTCR have to be pre-treated by firing them for 2 hours at 600°C in air. After this pre-treatment the PTCR will maintain its full capability without any exception (we advise to contact our customer service desk before using the PTCR in these conditions).

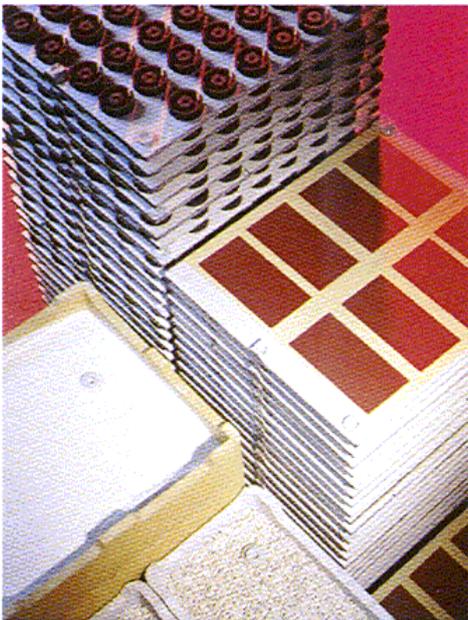

8. Is the performance of the PTCR influenced by the atmospheric conditions?

Yes, the actual atmospheric conditions have an influence on the rate of contraction of the ring. This leads to a RT reading, which may differ from the expected value, e.g. it may be lower. This however has no influence on the reproducibility of the reading, which will still assure the firing conditions to be within the process limits.

9. How is the performance of PTCR affected by the soak time?

The PTCR will continue to contract as long as it is exposed to heat. Effectively this means that at a constant set temperature, the RT reading will be higher, the longer the soak time is.

No, provided the table delivered with a new batch is used, no changes to the settings are necessary. Every new batch of PTCR is factory (re)calibrated to assure the same RT reading under the same kiln conditions.

11. Is there any influence of the material of the supports used?

Yes, it is known that "reactive" support material like e.g. carbon strongly inhibits the performance of ceramic temperature indicators. The support should be of a non reactive material, like ZrO<sub>2</sub>, Al<sub>2</sub>O<sub>3</sub>, SiN etc.

12. Has the temperature ramp-up any influence on the PTCR performance?

Yes it does, because the PTCR registers the cumulative amount of heat absorbed, a long ramp-up time will result in a higher RT reading than a fast temperature ramp-up.

13. Do I need the micrometer to perform the measurements?

To ensure a correct determination of the contraction of the ring, it is of vital importance, that the ring is positioned correctly during the measurement of the ring diameter after the firing cycle is completed. The special measuring device is the best assurance of a correct "foolproof" RT reading.

14. Why do different batches yield different ring temperatures and how are these differences compensated for?

Batches differ, there is no question about that, there is no avoiding that. The reason for this is that the materials used to manufacture the rings differ from batch to batch. There are differences in composition, grain size distribution and so on, which affect the shrinkage of the rings made with these materials. So even though the same recipe is used with every batch, there will be small but significant differences.

To compensate for these differences a calibration of each batch by firing rings from the new batch together with rings from the reference batch in their standard conditions can be done. Usually slightly different diameters are found. The diameter from the reference rings gives the actual temperature.

The diameter from the rings of the new batch is correlated to this temperature. This process is repeated 8 times, each time at a different temperature, covering the entire temperature range of the rings. This results in 8 diameters, which correlate to 8 actual temperatures. A curve is fitted through these 8 points, which is used to make the new table. For the standard conditions the differences in shrinkage between the new batch and the reference batch now have been compensated for.

Firing under different conditions (different curve, different atmosphere, etc.) might not have exactly the same effect on rings from different batches. When this is the case, the compensation introduced must be altered in order to achieve the exact same ring temperature with different batches of rings. This is not a bad thing. It is just a modification of the

calibration to suit a specific firing process. Theoretically, the rings should be re-calibrated for each process every time a new batch is used. As a service to customers a "standard" compensation, which works very well for most processes can be provided. Occasionally, differences between batches when fired with a specific firing process get too great or a customer wants the highest possible degree of accuracy. The customer then has to calibrate the new batch of rings himself.

